



R&S®FPL1-K54 EMI MEASUREMENT APPLICATION

Detecting and eliminating electromagnetic interference

The perfect choice for



Max. peak detector-based signal sweep (top) and quasi-peak detector-based disturbance maxima analysis (bottom)

Detecting and eliminating electromagnetic interference

The R&S®FPL1-K54 EMI measurement application adds EMI diagnostic functionality to the R&S®FPL signal and spectrum analyzer. It is the ideal tool for debugging and precompliance applications.

- ▶ Emission measurements in line with EMI standards
- ▶ Extensive limit line library for quick pass/fail decisions
- ▶ Transducer factor library with correction value tables for EMI accessories (LISNs, antennas, clamps, preamplifiers, cables and attenuators)

Detection and analysis of unwanted emissions (radiated or conducted)


EMI precompliance testing in line with commercial, automotive, avionic and military standards (CISPR, EN, FCC, DO-160, MIL-STD-461)

- ▶ Remote control of line impedance stabilization networks (LISN) from Rohde & Schwarz with the R&S®FPL1-B5 option
- ▶ Acoustic analysis using FM and AM signal demodulation with the R&S®FPL1-B5 option
- ▶ Logarithmic spectrum display
- ▶ Measurement automation: signal sweep with max. peak detector and subsequent disturbance maxima analysis with CISPR detectors

Key specifications	
EMI filters (6 dB)	CISPR 16-1-1: 200 Hz, 9 kHz, 120 kHz, 1 MHz MIL-STD-461: 10 Hz, 100 Hz, 1 kHz, 10 kHz, 100 kHz, 1 MHz
EMI detectors (CISPR 16-1-1)	quasi-peak, CISPR-average, RMS-average
Number of meas. markers	1 to 16

Your benefit	Features
Fast and reliable disturbance detection	automatic disturbance maxima detection and analysis with CISPR detectors
Smooth EMI certification process	RBWs and detectors in line with CISPR 16-1-1 and MIL-STD-461

Example of emission analysis: voltage mains measurement of a lamp

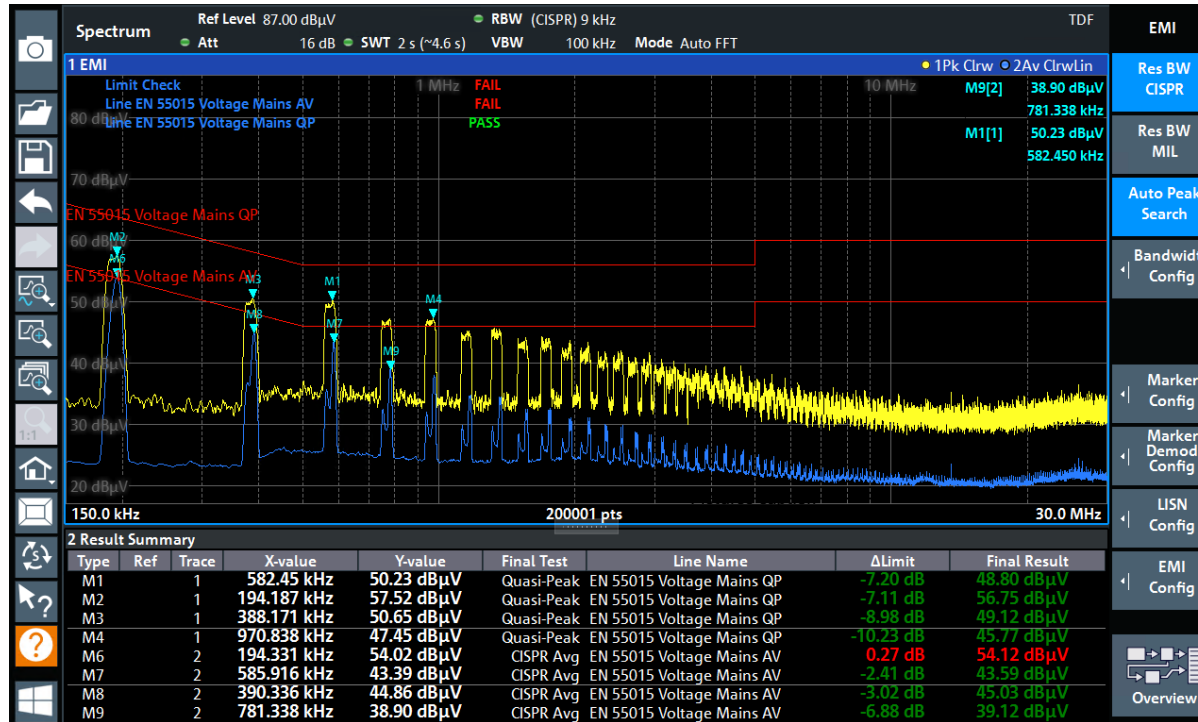

Two detectors are used for the sweep: positive peak (yellow curve) and average (blue curve). Pass/fail information is given according to the defined limits (red lines). The identified maxima ("Auto Peak Search") are automatically measured using the related CISPR detectors (quasi-peak and average) and listed in the results table. The final pass/fail status is clearly shown. The R&S®FPL applies the correction values (transducer factor) of the used LISN to the measurement results.

Model configuration information	
Description	Item
Signal and spectrum analyzer, 5 kHz to 3 GHz	R&S®FPL1003
Signal and spectrum analyzer, 5 kHz to 7.5 GHz	R&S®FPL1007
Required options	
EMI measurement application	R&S®FPL1-K54
Additional interfaces (required for audio demodulation and LISN remote control)	R&S®FPL1-B5
Recommended option	
RF preamplifier	R&S®FPL1-B22

Rohde & Schwarz Representative

Thurlby Thandar Instrument Distribution
Glebe Road, Huntingdon, PE29 7DR, UK
+44 (0)1480 412 451
sales@ttid.co.uk
www.ttid.co.uk

TTid.co.uk
THURLBY THANDAR
instrument distribution

Rohde & Schwarz GmbH & Co. KG | Europe, Africa, Middle East +49 89 4129 12345 | North America 1 888 TEST RSA (1 888 837 87 72)
Latin America +1 410 910 79 88 | Asia Pacific +65 65 13 04 88 | China +86 800 810 82 28 / +86 400 650 58 96
www.rohde-schwarz.com | customersupport@rohde-schwarz.com

R&S® is a registered trademark of Rohde & Schwarz GmbH & Co. KG | PD 3609.1762.32 | Version 01.01 | March 2019 (tt)
Trade names are trademarks of the owners | R&S®FPL1-K54 EMI measurement application | Data without tolerance limits is not binding
Subject to change | © 2019 Rohde & Schwarz GmbH & Co. KG | 81671 Munich, Germany